

## TGS 2444 - for the detection of Ammonia

### Features:


- \* Low power consumption
- \* High sensitivity/selectivity to ammonia (NH<sub>3</sub>)
- \* Miniature size

### Applications:

- \* Ammonia leak detection in refrigerators
- \* Ventilation control for agricultural and poultry industries


**TGS 2444** utilizes a multilayer sensor structure. A glass layer for thermal insulation is printed between a ruthenium oxide (RuO<sub>2</sub>) heater and an alumina substrate. A pair of Au electrodes for the heater are formed on a thermal insulator. The gas sensing layer, which is formed of tin dioxide (SnO<sub>2</sub>), is printed on an electrical insulation layer which covers the heater. A pair of Au electrodes for measuring sensor resistance are formed on the electrical insulator.

**TGS 2444** displays good selectivity to ammonia, making it ideal for critical safety-related applications such as the detection of ammonia leaks in refrigeration systems and ammonia detection in the agricultural field. In the presence of ammonia, the sensor's conductivity increases depending on the gas concentration in the air. A simple pulsed electrical circuit operating on a 250msec circuit voltage cycle can convert the change in conductivity to an output signal which corresponds to gas concentration.




The figure below represents typical sensitivity characteristics, all data having been gathered at standard test conditions (see reverse side of this sheet). The Y-axis is indicated as sensor resistance of displayed gases at various concentrations:

### Sensitivity Characteristics:



The figure below represents the typical response pattern of TGS2444 when the atmosphere changes from clean air to the listed gas concentrations and then reverts back to clean air:

### Sensor Response Pattern:

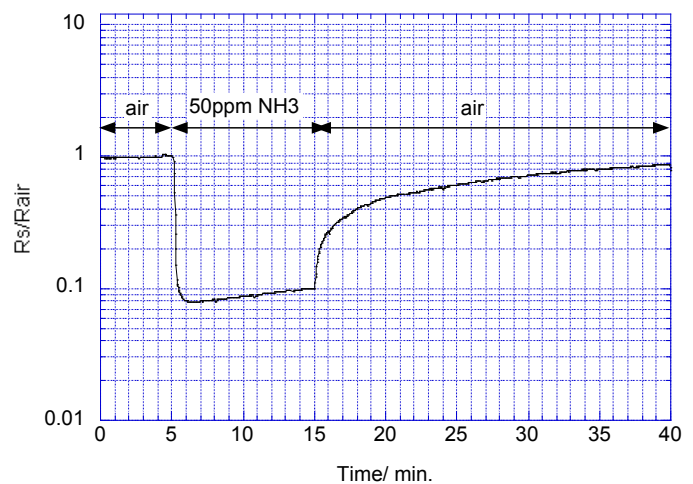

**ApolloSense Ltd**

Shenzhen:

Address : Room 712, Huaneng Building, Shennan Zhong Road, Shenzhen 518031, China

Tel : ( 86-755 ) 83680810 83680820 83680830 83680860

Fax : ( 86-755 ) 83680866

Hong Kong:

Address : Unit 1502, Hollywood Plaza, 610 Nathan Road, Mong Kok, Kln., H.K.

Tel : (852) 2737 0903

Fax : (852) 2737 0938

Email : sales@apollounion.com



## Basic Measuring Circuit:

Circuit voltage ( $V_C$ ) is applied across the sensing element which has a resistance ( $R_S$ ) between the sensor's two electrodes (pins No. 2 and No. 3) and a load resistor ( $R_L$ ) connected in series. The sensing element is heated by the heater which is connected to pins No. 1 and No. 4.


**Heating cycle**--The sensor requires application of a 250 msec heating cycle which is used in connection with a circuit voltage cycle of 250 msec. Each  $V_H$  cycle is comprised of 4.8V being applied to the heater for the first 14ms, followed by 0V pulse for the remaining 236ms. The  $V_C$  cycle consists of 0V applied for 2msec, followed by 5.0V for 5ms and 0V for 243msec. For achieving optimal sensing

characteristics, the sensor's signal should be measured after the midpoint of the 5ms  $V_C$  pulse of 5.0V (for reference, see timing chart below).

**NOTE:** Application of a  $V_C$  pulse condition is required to prevent possible migration of heater materials into the sensing element material. Under extreme conditions of high humidity and temperature, a constant  $V_C$  condition could result in such migration and cause long term drift of  $R_S$  to higher values. A 5ms  $V_C$  pulse results in significantly less driving force for migration than a constant  $V_C$  condition, rendering the possibility of migration negligibly small.



## Structure and Dimensions:



Pin connections:

- 1: Heater
- 2: Sensor (-)
- 3: Sensor (+)
- 4: Heater

## Specifications:

Model number		TGS2444	
Sensing element type		M1	
Standard package		TO-5 metal can	
Target gases		Ammonia	
Typical detection range		10 ~ 300ppm	
Standard circuit conditions	Heater voltage cycle	$V_H$	$V_{HH}=4.8V \pm 0.2VDC$ for 14ms $V_{HL}=0V$ for 236ms
	Circuit voltage cycle	$V_C$	$V_C=0V$ for 245ms $V_C=5.0V \pm 0.2VDC$ for 5ms (see timing chart for measurement timing)
	Load resistance	$R_L$	variable $R_L \geq 8k\Omega$
Electrical characteristics under standard test conditions	Heater resistance	$R_H$	$17 \pm 2.5\Omega$ at room temp.
	Heater current	$I_H$	approx. 203mA (in case of $V_{HH}$ )
	Heater power consumption	$P_H$	56mW (typical)
	Sensor resistance	$R_S$	$2.0k\Omega \sim 40.6k\Omega$ in 30ppm of ammonia
	Sensitivity (change ratio of $R_S$ )	$\beta$	$\frac{R_S(NH_3 \ 100ppm)}{R_S(NH_3 \ 30ppm)}$ 0.08 ~ 0.84
Standard test conditions	Test gas conditions	Ammonia in air at $20 \pm 2^\circ C$ , $65 \pm 5\% RH$	
	Circuit conditions	Same as Std Circuit Condition (above)	
	Conditioning period before test	$\geq 48$ hours	
Operating conditions	$-40^\circ C \sim +50^\circ C$ w/o dew condensation Less than absolute humidity corresponds to $40^\circ C/50\% RH$		
Storage conditions	$-40^\circ C \sim +60^\circ C$ w/o dew condensation Less than absolute humidity corresponds to $60^\circ C/70\% RH$		

Sensor resistance ( $R_S$ ) is calculated with a measured value of  $V_{out}$  as follows:

$$R_S = \frac{V_C \times R_L}{V_{out}} - R_L$$

## ApolloSense Ltd